

GUIDED SURGERY

ELEMENT & CONTACT PF 3.5-PF 4.5 / L 6.5-L 12.5, ALL COLLARS



MONO torque ratchet*

Titanium alloy



MONO guide key*

Stainless steel



Guide sleeve

Stainless steel



Seating instrument for guide sleeves

Stainless steel




Lenght mm 5.0
Ø 4.8 3.04.080 Q4

Ø 4.8 3.04.100

Cassette for guided surgery 1.04.020

⚠ Specific slots are provided for loading of the instruments. Refer to dental shaft and graphic insert.

Example:

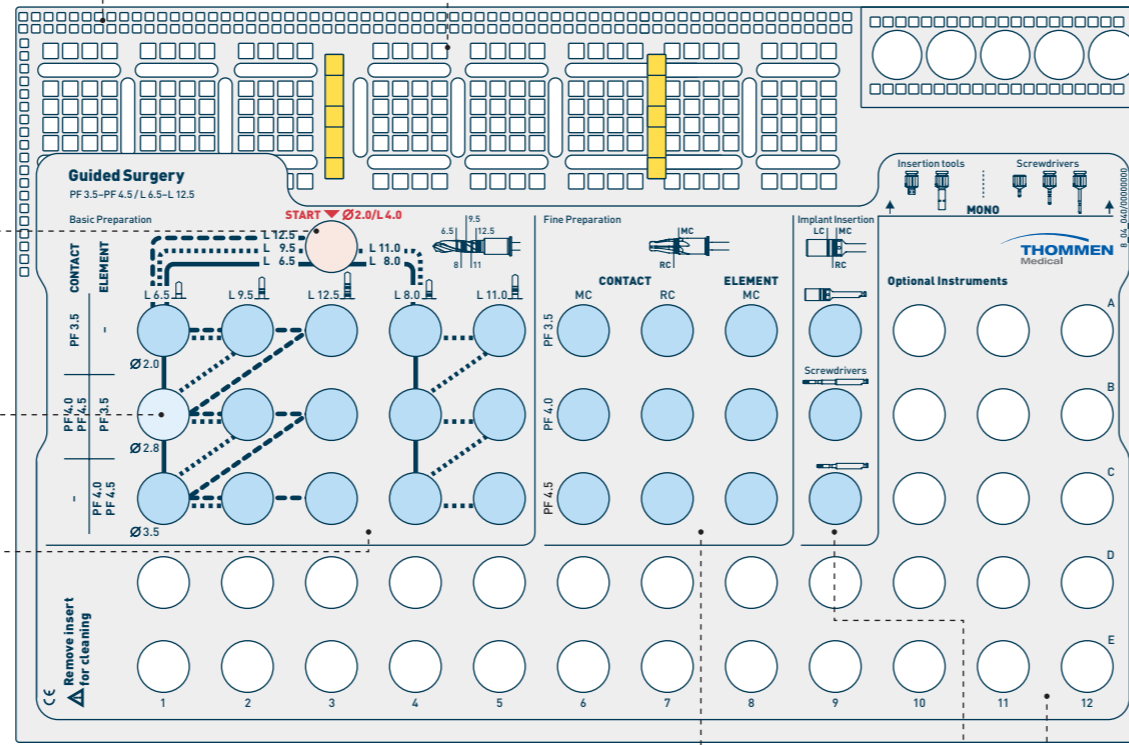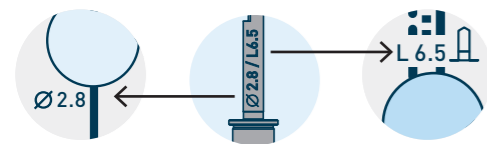

MONO insertion device*

Stainless steel/PEEK

3.03.162 3.03.163

MONO screwdriver*


Stainless steel/PEEK

3.03.165 3.03.166 3.03.167



Ø 2.0 / L 4.0

800 rpm



Basic preparation initial drill, guided


Stainless steel

	L 4.0
Lenght mm	28.5
Ø 2.0	3.04.110



Ø 2.0 Ø 2.8 Ø 3.5

800 rpm 600 rpm 500 rpm



Basic preparation VECTOdriLL™ pilot drill and twist drills, guided


Stainless steel

	L 6.5	L 9.5	L 12.5	L 8.0	L 11.0
Lenght mm	31.5	34.5	37.5	33.0	36.0
Ø 2.0	3.04.111	3.04.113	3.04.115	3.04.112	3.04.114
Ø 2.8	3.04.121	3.04.123	3.04.125	3.04.122	3.04.124
Ø 3.5	3.04.131	3.04.133	3.04.135	3.04.132	3.04.134



Ø 2.0 / L 4.0

250 rpm




Fine preparation profile drills, guided

Stainless steel

	CONTACT MC	CONTACT RC	ELEMENT MC
Lenght mm	34.0	32.5	30.5
Ø 3.5	3.04.171	3.04.161	3.04.151
Ø 4.0	3.04.172	3.04.162	3.04.152
Ø 4.5	3.04.173	3.04.163	3.04.153

15 rpm



Implant Insertion adapter, guided

Stainless steel


	Adapter, guided	Screwdriver, short	Screwdriver, extra short
Lenght mm	25.5	22.0	17.0
	3.04.090	3.03.501	3.03.500



Max. 20 application cycles (surgery, cleaning, sterilization) for cutting instruments. Further application cycles do not guarantee the function of the product anymore.



Cooling during irrigation, approx 5° C / 41 °F.



Optional Instruments*

Along with the clearly designated slots, additional slots are provided that can be loaded as required.

* Standard instruments (refer to www.ifu-tm.com/THM61141)